


Disclaimer




- NIST falls within the Department of Commerce
 - Mission: to promote innovation and industrial competitiveness by advancing measurement science, standards, and technology
- Our focus is on making measurements
 - Robust examinations of technology
 - Collaboration with other federal/state/local users
 - · Collaboration with industry
- NIST is not a consumer reports agency for commercial products

2018 Rapid DNA Maturity Assessment

- Goal: To measure the status of rapid DNA typing technology for the 20 CODIS core loci in support of booking station Rapid DNA implementation
- Rapid DNA instruments capable of genotyping the 20 CODIS core loci were eligible for participation
- 20 single source reference buccal swabs were distributed to participating laboratories

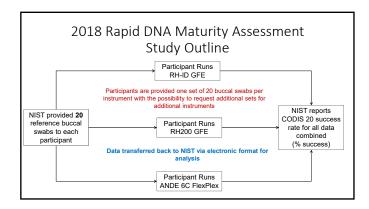

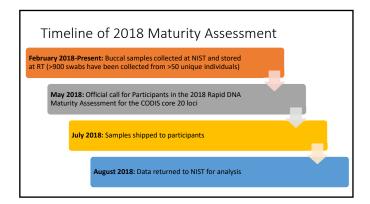

20 Swabs provided Participants	Instrument Platforms	Chemistry	Independent Instruments	Total Samples Tested	Analysis Method
Federal	ANDE 6C	FlexPlex	5	100	Rapid DNA Analysis
State Police	IntegenX RapidHIT 200	GlobalFiler Express	3	60	Modified Rapid DNA Analysis
Vendor	IntegenX RapidHIT ID	GlobalFiler Express	4	80	Modified Rapid DNA Analysis
9 Participants	3 Platforms		12 Instruments	240 Sample	S

Success Metrics

- Success was measured by complete and concordant genotypes produced for the 20 CODIS core loci
- Allele calls by the integrated rapid DNA devices were compared to lab generated profiles for concordance
 - Fusion 6C, PP21, GFE on a 3500xL
- \bullet Two interpretation parameters were implemented
 - Rapid DNA Analysis: Without human intervention
 - Modified Rapid DNA Analysis: Expert interpretation and analysis of electropherogram

https://www.fhi.gov/file-renository/addendum-to-pas-for-rapid-doa.ndf/view

Rapid DNA Analysis-ANDE

Automated (lights-out) analysis without human intervention


Effective June 1, 2018, the following Ropid DNA system is approved for use at NDIS by an accredited foreisic DNA laboratory.

Rapid DNA Analysis System for Accredited Laboratory Use

To date, ANDE 6C is the only rapid DNA system to be NDIS approved for automated rapid DNA analysis


Component	Name	Part/Version Number
Rapid DNA Instrument	ANDE 6C Instrument	A0120001003
Typing Kit	FlexPiex27	FlexPiex27
Cartridge	ANDE A-Chip (FlexPlex)	AG210001057
System Software	ANDE System Software	2.0.6
Expert System Software	ANDE Expert System	205


https://www.fbi.gov/services/laboratory/biometric-analysis/codis/rapid-dna

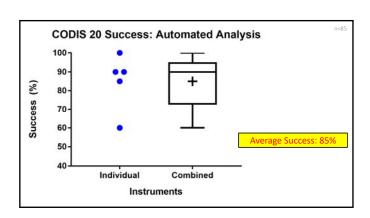



Modified Analysis Parameters


- Samples were manually reviewed (n=240)
 - ANDE profiles were analyzed in GeneMapper IDX v1.5
 - RapidHIT profiles were reviewed in GeneMarker HID v2.8.2
 - Heterozygote balance filter set at 0.25
- After manually interpreting a profile (PHR >0.25, low AT, recovery of "lost" data), concordance was checked against the laboratory generated reference profile
- Success was determined by complete and concordant profiles for the 20 CODIS core loci

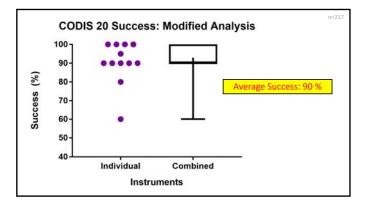


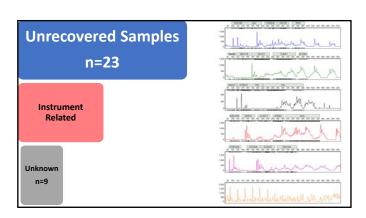

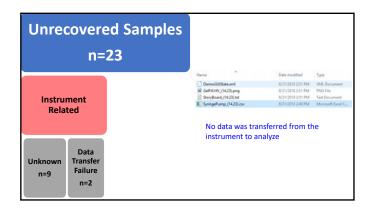

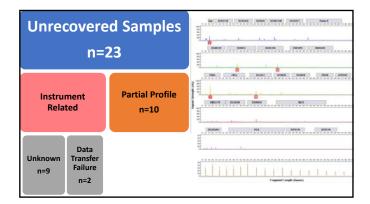

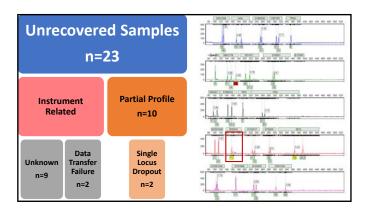


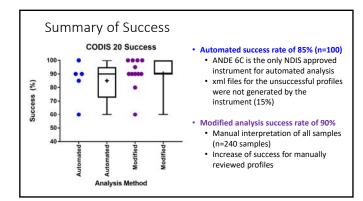



n=217 successful profiles


Additional Metrics Analyzed


Base pair sizing precision Heterozygote Balance

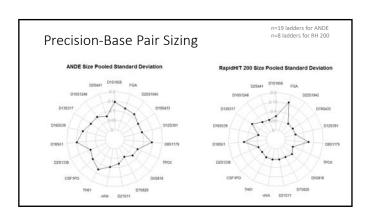

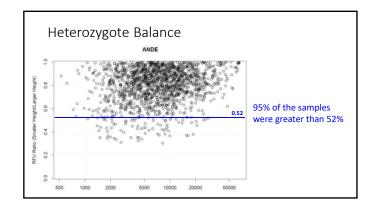

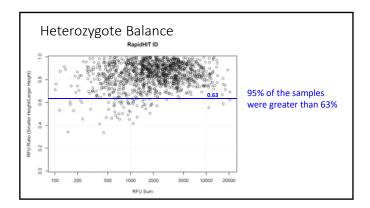

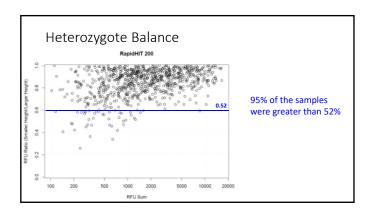

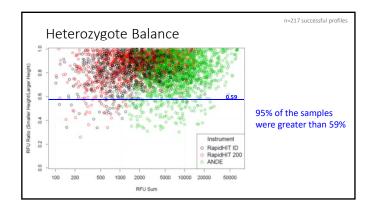

Maturity Assessment Summary

- 12 instruments tested across 9 laboratories
- Total of 240 samples examined
 - 85% success rate for the CODIS 20 using Rapid DNA Analysis
 - 90% success rate for the CODIS 20 using Modified Rapid DNA Analysis
 - Success ranged from 60% to 100%
 - Precision was below 0.17 bp on for both ANDE 6C and RapidHIT 200
 - Combined heterozygote balance (all three instruments) was above 59%

Thank you to our participants

- ANDE
- Arizona Department of Public Safety
- Bensalem Police Department
- Federal Bureau of Investigation Laboratory
- Louisiana State Police Crime Laboratory
- Miami Beach Police Department
- Miami Dade Police Department
- NIST (DHS instruments, run at SNA Intl.)
- U.S. Army Criminal Investigation Laboratory





Acknowledgements

Save the Date!



NIST – Applied Genetics Group Peter Vallone Steven Lund

Funding
FBI Biometrics Center of Excellence: Forensic
DNA Typing as a Biometric tool.

Contact Information erica.romsos@nist.gov

Rapid DNA Instrument	Number of Total Instruments Participating Labs		Samples Attempted	CODIS Success (Rapid DNA Analysis)	CODIS Success (Modified Rapid DNA Analysis)
3	9	12	240	85%	90%